


Certificate of Analysis


Oil Distributors Ltd
Blend 1: TB500 + BPC157

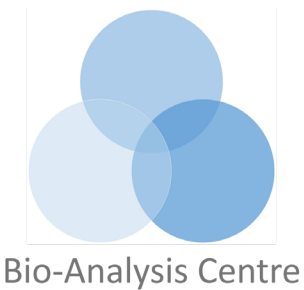

Analysis Method:

Sample Preparation	Dissolved in water (2ml)			
Instrument	Shimadzu Nexera HPLC	Injection Volume	5µl	
Column	Zorbax Extend C18	Analysis wavelength	215nm	
Column Dimensions	4.6 x 150 mm	Run time	30 mins	
Guard Column	Yes	Gradient	Time (min)	%B
Mobile Phase A	0.1% Formic Acid in Water		0 - 0.5	2
Mobile Phase B	0.1% Formic Acid in Acetonitrile		0.5 - 20.5	2 - 30
Flow	1 ml/min		20.5 - 20.6	30 - 95
Column Temperature	40°C		20.6 - 25.5	95
Autosampler temperature	15°C		25.5 - 25.7	95 - 2

Datafile Name:20251010 batch8_Blend 1_TBC500+BP157_005.lcd
Sample Name:Blend 1
Sample ID:TBC500+BP157

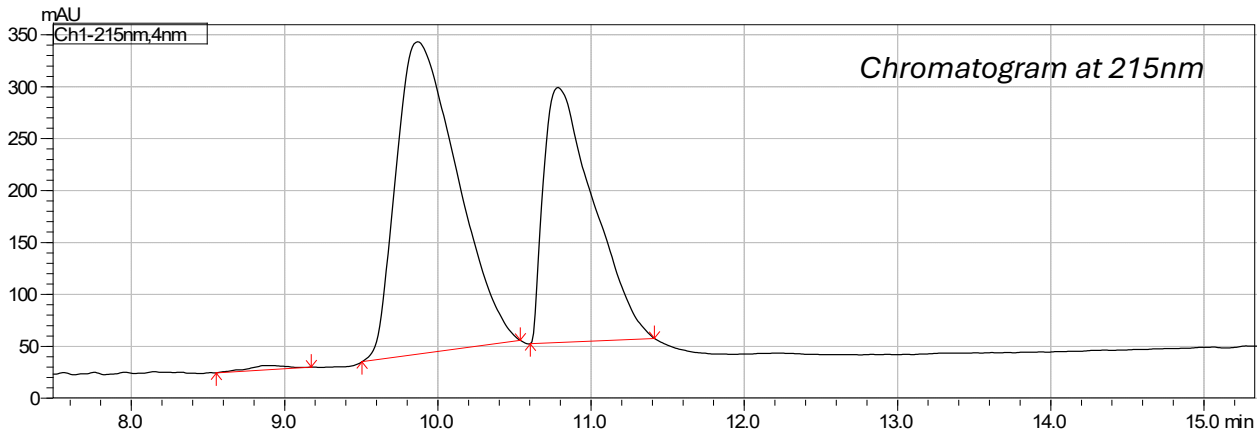

Peak Table

Peak#	Ret. Time	Area	Area%	Peak Purity Index	% Purity
1	8.864	68883	0.493	0.99922	99.92
2	9.867	8323742	59.59	0.99232	99.23
3	10.78	5575885	39.92	0.99153	99.15

Peak Purity Graph

