


Certificate of Analysis


Oil Distributors Ltd
K-Glow

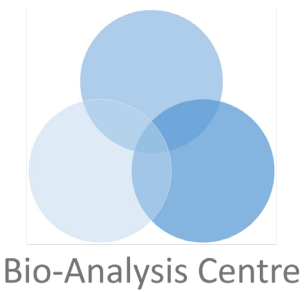

Analysis Method:

Sample Preparation	Dissolved in water (2ml)			
Instrument	Shimadzu Nexera HPLC	Injection Volume	5µl	
Column	Zorbax Extend C18	Analysis wavelength	215nm	
Column Dimensions	4.6 x 150 mm	Run time	30 mins	
Guard Column	Yes	Gradient	Time (min)	%B
Mobile Phase A	0.1% Formic Acid in Water		0 - 0.5	2
Mobile Phase B	0.1% Formic Acid in Acetonitrile		0.5 - 20.5	2 - 30
Flow	1 ml/min		20.5 - 20.6	30 - 95
Column Temperature	40°C		20.6 - 25.5	95
Autosampler temperature	15°C		25.5 - 25.7	95 - 2

Datafile Name:20251010_batch8_K-Glow_BPC+TB500+GHKCu+KPV_002.lcd
Sample Name:K-Glow
Sample ID:BPC+TB500+GHKCu+KPV

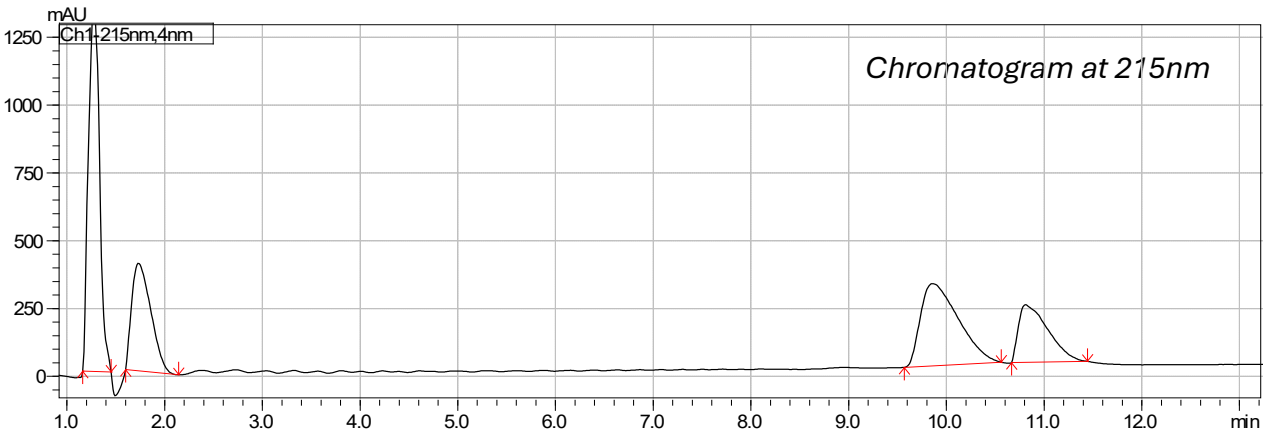

Peak Table

Peak#	Ret. Time	Area	Area%	Peak Purity Index	% Purity
1	1.269	10781231	37.42	0.98034	98.03
2	1.739	5414145	18.79	0.99509	99.51
3	9.856	8160947	28.32	0.99007	99.01
4	10.81	4458143	15.47	0.98832	98.83

Peak Purity Graph

