


Certificate of Analysis

Oil Distributors Ltd
Sermorelin




Bio-Analysis Centre

Analysis Method:

Sample Preparation	Dissolved in water (2ml)			
Instrument	Shimadzu Nexera HPLC	Injection Volume	1µl	
Column	Zorbax Extend C18	Analysis wavelength	215nm	
Column Dimensions	4.6 x 150 mm	Run time	15 mins	
Guard Column	Yes	Gradient	Time (min)	%B
Mobile Phase A	0.1% Formic Acid in Water		0 - 0.5	20
Mobile Phase B	0.1% Formic Acid in Acetonitrile		0.5 - 10.5	20 - 60
Flow	1 ml/min		10.5 - 10.6	60 - 95
Column Temperature	40°C		10.6 - 12.6	95
Autosampler temperature	15°C		12.6 - 12.7	95 - 20

Datafile Name:20251002 batch 1_sermorelin__029.lcd
Sample Name:sermorelin

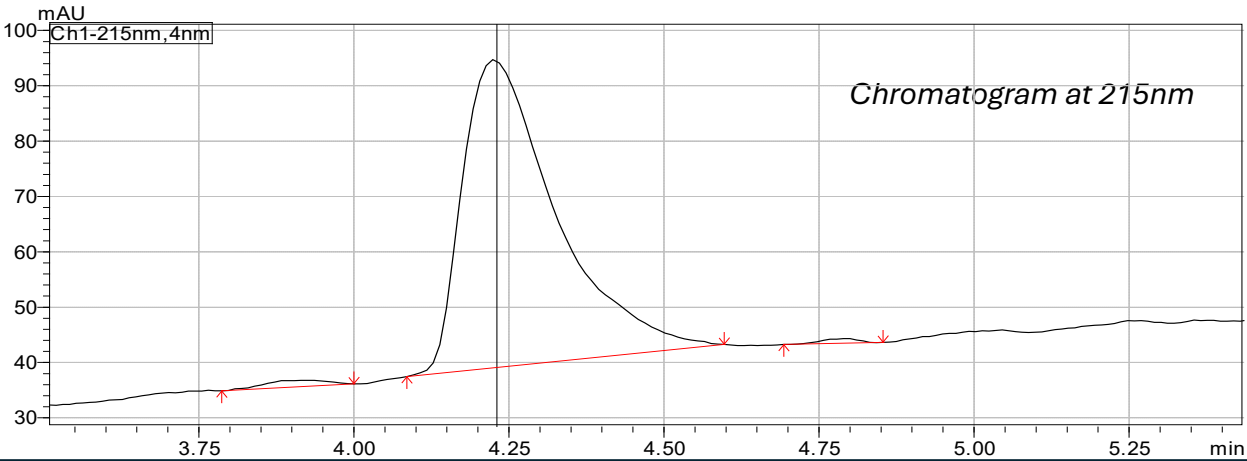

Peak Table

Peak#	Ret. Time	Area	Area%	Peak Purity Index
1	3.883	8652	1.456	0.99971
2	4.224	582348	97.976	0.979462
3	4.789	3378	0.568	0.999942

Overall Purity **96.0%**

Peak Purity Graph

